

CALIBRATION LABORATORIES

NVLAP LAB CODE 200127-0

SCOPE OF ACCREDITATION TO ISO/IEC 17025:2017


<p>David L. Ellis Co., Incorporated 310 Old High Street, P.O. Box 592 Acton, MA 01720-0010 Mr. Robert A. Ellis Phone: 978-897-1795 Fax: 978-897-0844 E-mail: sales@hardness-testblocks.com URL: http://www.hardness-testblocks.com</p>	<p>Fields of Calibration Mechanical</p> <p>This laboratory is compliant to ANSI/NCSL Z540-1-1994; Part 1. (NVLAP Code: 20/A01)</p>
---	--

CALIBRATION AND MEASUREMENT CAPABILITIES (CMC)^{Notes 1,2,11}

Measured Parameter or Device Calibrated	Range	Expanded Uncertainty ^{Note 3}	Remarks
MECHANICAL			
HARDNESS (20/M13)			
Calibration of Test Blocks Rockwell ASTM E18, ISO 6508			See notes 7, 8, and 9
HRA Scale	≥ 86	0.17	Uncertainty given in Rockwell points
	80 to 85	0.17	
	70 to 79	0.29	
	60 to 69	0.28	
HRB Scale	≥ 80	0.37	
	51 to 79	0.24	
	1 to 50	0.33	
HRC Scale	60 to 70	0.31	
	40 to 59	0.32	
	20 to 39	0.37	
HRD Scale	70 to 80	0.17	
	50 to 69	0.26	
	40 to 49	0.24	
HRE Scale	≥ 89	0.48	
	75 to 88	0.48	
	65 to 87	0.36	
HRF Scale	≥ 87	0.44	
	70 to 86	0.45	
	40 to 69	0.25	

2020-09-18 through 2021-09-30

Effective dates



For the National Voluntary Laboratory Accreditation Program

CALIBRATION LABORATORIES


NVLAP LAB CODE 200127-0

CALIBRATION AND MEASUREMENT CAPABILITIES (CMC)^{Notes 1,2,11}

Measured Parameter or Device Calibrated	Range	Expanded Uncertainty ^{Note 3}	Remarks
HRG Scale	≥ 80	0.23	
	40 to 79	0.17	
	1 to 39	0.76	
HRH Scale	≥ 90	0.35	
	80 to 89	0.41	
	60 to 79	0.71	
HRK Scale	≥ 70	0.34	
	30 to 69	0.47	
	10 to 29	0.54	
HRL Scale	≥ 115	0.17	
	90 to 114	0.24	
HRM Scale	≥ 100	0.41	
	70 to 99	0.52	
HRP Scale	≥ 85	0.34	
	40 to 84	0.50	
HRR Scale	≥ 120	0.22	
	100 to 119	0.33	
HRS Scale	≥ 112	0.17	
	110 to 111	0.78	
HRV Scale	≥ 104	0.25	
	80 to 103	0.21	
HR15N Scale	90 to 95	0.50	
	80 to 89	0.40	
HR15T Scale	40 to 79	0.39	
	88 to 100	0.29	
	80 to 87	0.36	
HR15W Scale	20 to 79	0.41	
	89 to 100	0.42	
HR15X Scale	80 to 88	0.24	
	88 to 100	0.17	
HR15Y Scale	80 to 87	0.54	
	94 to 100	0.20	
HR30N Scale	85 to 93	0.44	
	77 to 85	0.52	
	60 to 76	0.45	
	40 to 59	0.26	

2020-09-18 through 2021-09-30

Effective dates

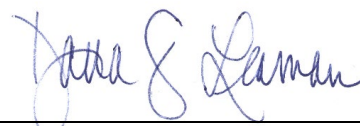

For the National Voluntary Laboratory Accreditation Program

CALIBRATION LABORATORIES


NVLAP LAB CODE 200127-0

CALIBRATION AND MEASUREMENT CAPABILITIES (CMC)^{Notes 1,2,11}

Measured Parameter or Device Calibrated	Range	Expanded Uncertainty ^{Note 3}	Remarks
HR30T Scale	57 to 85	0.19	See notes 7 and 8. Range and uncertainty given in Rockwell points
	50 to 56	0.62	
	20 to 49	0.55	
HR30W Scale	65 to 100	0.31	
	40 to 64	0.81	
HR30X Scale	79 to 100	0.17	
	60 to 78	0.95	
HR30Y Scale	88 to 100	0.31	
	60 to 87	0.20	
HR45N Scale	67 to 75	0.17	
	50 to 66	0.21	
	10 to 49	0.47	
HR45T Scale	50 to 75	0.37	
	40 to 49	0.38	
	1 to 39	0.68	
HR45W Scale	49 to 100	0.28	
	10 to 47	0.75	
HR45X Scale	69 to 100	0.17	
	40 to 68	0.74	
HR45Y Scale	82 to 100	0.22	
	60 to 81	0.62	
Field Service ^{Note 4} Indirect Verification of Hardness Testing Machines Rockwell ASTM E18, ISO 6508			
HR15N Scale	90 to 95	0.50	
	80 to 89	0.41	
	40 to 79	0.40	
HR15T Scale	≥ 88	0.42	
	80 to 87	0.51	
	20 to 79	0.60	
HR15W Scale	≥ 89	0.61	
	80 to 88	.036	
HR15X Scale	≥ 88	0.18	
	80 to 87	0.55	

2020-09-18 through 2021-09-30

Effective dates



For the National Voluntary Laboratory Accreditation Program

CALIBRATION LABORATORIES


NVLAP LAB CODE 200127-0

CALIBRATION AND MEASUREMENT CAPABILITIES (CMC)^{Notes 1,2,11}

Measured Parameter or Device Calibrated	Range	Expanded Uncertainty^{Note 3}	Remarks
HR15Y Scale	≥ 94	0.22	
	85 to 93	0.45	
HR30N Scale	77 to 85	0.53	
	60 to 76	0.46	
	40 to 59	0.28	
HRT30T Scale	≥ 57	0.21	
	50 to 56	0.63	
HR30W Scale	20 to 49	0.56	
	≥ 65	0.33	
HR30X Scale	40 to 64	0.82	
	≥ 79	0.19	
HR30Y Scale	60 to 78	0.95	
	≥ 88	0.33	
HR45N Scale	60 to 87	0.22	
	67 to 75	0.19	
	50 to 66	0.23	
HR45T Scale	10 to 49	0.48	
	≥ 50	0.38	
	40 to 49	0.39	
HR45W Scale	1 to 39	0.69	
	≥ 48	0.30	
HR45X Scale	10 to 47	0.76	
	≥ 69	0.18	
HR45Y Scale	40 to 68	0.75	
	≥ 82	0.24	
HRA Scale	60 to 81	0.63	
	≥ 86	0.18	
	80 to 85	0.18	
HRB Scale	70 to 79	0.23	
	60 to 69	0.29	
	≥ 80	0.38	
HRC Scale	51 to 79	0.26	
	1 to 50	0.34	
	60 to 70	0.32	
	40 to 59	0.34	
	20 to 39	0.38	

2020-09-18 through 2021-09-30

Effective dates

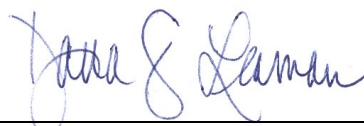


For the National Voluntary Laboratory Accreditation Program

CALIBRATION LABORATORIES

NVLAP LAB CODE 200127-0

CALIBRATION AND MEASUREMENT CAPABILITIES (CMC)^{Notes 1,2,11}

Measured Parameter or Device Calibrated	Range	Expanded Uncertainty ^{Note 3}	Remarks
HRD Scale	70 to 80	0.22	
	50 to 69	0.26	
	40 to 49	0.25	
HRE Scale	≥ 89	0.50	
	75 to 88	0.50	
	65 to 87	0.37	
HRF Scale	≥ 87	0.45	
	70 to 86	0.65	
	40 to 69	0.27	
HRG Scale	≥ 80	0.25	
	40 to 79	0.20	
	1 to 39	0.77	
HRH Scale	≥ 90	0.36	
	80 to 89	0.42	
	60 to 79	0.72	
HRK Scale	≥ 70	0.35	
	30 to 69	0.48	
	10 to 29	0.55	
HRL Scale	≥ 115	0.19	
	90 to 114	0.26	
	70 to 99	0.53	
HRM Scale	≥ 100	0.42	
	70 to 99	0.53	
	40 to 84	0.51	
HRP Scale	≥ 85	0.35	
	40 to 84	0.51	
	100 to 119	0.34	
HRR Scale	≥ 120	0.24	
	100 to 119	0.34	
	110 to 111	0.77	
HRS Scale	≥ 112	0.18	
	110 to 111	0.77	
	80 to 103	0.61	
HRV Scale	≥ 104	0.21	
	80 to 103	0.61	
	Rockwell Ball Indenters	Ball protrusion 1/16", 1/8", 1/4", 1/2"	0.004 mm
Hardness ball holder		1.2 HV10 (Vickers)	

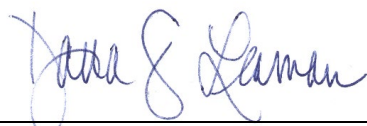

2020-09-18 through 2021-09-30

Effective dates

For the National Voluntary Laboratory Accreditation Program

CALIBRATION LABORATORIES


NVLAP LAB CODE 200127-0

CALIBRATION AND MEASUREMENT CAPABILITIES (CMC)^{Notes 1,2,11}

Measured Parameter or Device Calibrated	Range	Expanded Uncertainty ^{Note 3}	Remarks
	Performance 1/16" ball holder	0.25 HRBW	ASTM E18
	Performance 1/8" ball holder	0.30 HREW	ASTM E18
	Performance 1/4" ball holder	0.31 HRLW	ASTM E18
	Performance 1/2" ball holder	0.20 HRRW	ASTM E18
Calibrate Reference Test Blocks Brinell ASTM E10, ISO 6506 Brinell Scale			See notes 7, 8, and 10 Range in Brinell units
HBW 1/1	45 to 200	0.54 HBW	
HBW 1/1.25	200 to 400	9.5 HBW	
HBW 1/2.5	8.0 to 54.5	0.1 HBW	
HBW 1/5	15.9 to 109	0.1 HBW	
HBW 1/10	31.8 to 218	0.2 HBW	
HBW 1/30	45 to 200	0.3 HBW	
HBW 1/30	200 to 400	2.2 HBW	
HBW 1/30	400 to 650	6.0 HBW	
HBW 2.5/6.25	3.2 to 21.8	0.1 HBW	
HBW 2.5/7.8	4.0 to 27.2	0.1 HBW	
HBW 2.5/15.625	8.0 to 54.5	0.1 HBW	
HBW 2.5/31.25	15.9 to 109	0.1 HBW	
HBW 2.5/62.5	31.8 to 218	0.2 HBW	
HBW 2.5/187.5	45 to 200	0.3 HBW	
HBW 2.5/187.5	200 to 400	1.3 HBW	
HBW 2.5/187.5	400 to 700	2.9 HBW	
HBW 5/25	3/2 to 21.8	0.1 HBW	
HBW 5/31.25	4.0 to 27.2	0.1 HBW	
HBW 5/62.5	7.96 to 54.5	0.1 HBW	
HBW 5/125	15.9 to 109	0.1 HBW	
HBW 5/250	31.8 to 218	0.2 HBW	
HBW 5/750	45 to 200	0.30 HBW	
HBW 5/750	200 to 400	1.8 HBW	
HBW 5/750	400 to 600	4.6 HBW	

2020-09-18 through 2021-09-30

Effective dates



For the National Voluntary Laboratory Accreditation Program

CALIBRATION LABORATORIES


NVLAP LAB CODE 200127-0

CALIBRATION AND MEASUREMENT CAPABILITIES (CMC)^{Notes 1,2,11}

Measured Parameter or Device Calibrated	Range	Expanded Uncertainty ^{Note 3}	Remarks
HBW 10/100	3.2 to 21.8	0.1 HBW	
HBW 10/125	4.0 to 27.2	0.1 HBW	
HBW 10/250	8.0 to 54.5	0.1 HBW	
HBW 10/500	100 to 150	0.30 HBW	
HBW 10/1000	45 to 200	0.40 HBW	
HBW 10/1000	200 to 400	1.4 HBW	
HBW 10/1500	45 to 200	0.3 HBW	
HBW 10/1500	200 to 400	1.5 HBW	
HBW 10/1500	400 to 700	3.5 HBW	
HBW 10/2000	45 to 200	0.3 HBW	
HBW 10/2000	200 to 400	1.4 HBW	
HBW 10/2000	400 to 700	3.2 HBW	
HBW 10/2500	45 to 200	0.3 HBW	
HBW 10/2500	200 to 400	1.3 HBW	
HBW 10/2500	400 to 700	3.0 HBW	
HBW 10/3000	45 to 200	0.3 HBW	
HBW 10/3000	200 to 400	1.3 HBW	
HBW 10/3000	400 to 700	2.9 HBW	
Vickers: ASTM E92, ASTM E384			See notes 7, 8, and 10 Range in Vickers units
HV 1	200 to 400	1.5 HV	
HV 1	400 to 700	3.6 HV	
HV 1	700 to 2 300	7.7 HV	
HV 1.5	25 to 200	0.1 HV	
HV 1.5	200 to 400	1.4 HV	
HV 1.5	400 to 700	3.2 HV	
HV 1.5	700 to 2 300	6.7 HV	
HV 2	25 to 200	0.1 HV	
HV 2	200 to 400	1.3 HV	
HV 2	400 to 700	3.0 HV	
HV 2	700 to 2 300	6.1 HV	
HV 2.5	25 to 200	0.1 HV	
HV 2.5	200 to 400	1.3 HV	
HV 2.5	400 to 700	2.9 HV	
HV 2.5	700 to 2300	5.7 HV	

2020-09-18 through 2021-09-30

Effective dates



For the National Voluntary Laboratory Accreditation Program

CALIBRATION LABORATORIES


NVLAP LAB CODE 200127-0

CALIBRATION AND MEASUREMENT CAPABILITIES (CMC)^{Notes 1,2,11}

Measured Parameter or Device Calibrated	Range	Expanded Uncertainty ^{Note 3}	Remarks
HV 3	25 to 200	0.1 HV	
HV 3	200 to 400	1.3 HV	
HV 3	400 to 700	2.8 HV	
HV 3	700 to 2300	5.5 HV	
HV 5	25 to 200	0.1 HV	
HV 5	200 to 400	1.2 HV	
HV 5	400 to 700	2.6 HV	
HV 5	700 to 2300	5.0 HV	
HV 10	25 to 200	0.1 HV	
HV 10	200 to 400	1.2 HV	
HV 10	400 to 700	2.5 HV	
HV 10	700 to 2300	4.5 HV	
HV 20	25 to 200	0.1 HV	
HV 20	200 to 400	1.2 HV	
HV 20	400 to 700	2.4 HV	
HV 20	700 to 2300	4.3 HV	
HV 30	25 to 200	0.1 HV	
HV 30	200 to 400	1.2 HV	
HV 30	400 to 700	2.3 HV	
HV 30	700 to 2300	4.2 HV	
HV 50	25 to 200	0.1 HV	
HV 50	200 to 400	1.2 HV	
HV 50	400 to 700	2.3 HV	
HV 50	700 to 2300	4.0 HV	
HV 100	25 to 200	0.1 HV	
HV 100	200 to 400	1.1 HV	
HV 100	400 to 700	2.3 HV	
HV 100	700 to 2300	4.0 HV	
Calibrate Reference Test Blocks Vickers: ASTM E384, ISO 6507 Vickers Scale			See notes 7, 8, and 10 Range in Vickers units
HV 0.01	25 to 200	0.5 HV	
HV 0.01	200 to 400	10 HV	
HV 0.01	400 to 700	28 HV	
HV 0.01	700 to 2300	64 HV	

2020-09-18 through 2021-09-30

Effective dates



For the National Voluntary Laboratory Accreditation Program

CALIBRATION LABORATORIES


NVLAP LAB CODE 200127-0

CALIBRATION AND MEASUREMENT CAPABILITIES (CMC)^{Notes 1,2,11}

Measured Parameter or Device Calibrated	Range	Expanded Uncertainty^{Note 3}	Remarks
HV 0.025	25 to 200	0.3 HV	
HV 0.025	200 to 400	6.4 HV	
HV 0.025	400 to 700	18 HV	
HV 0.025	700 to 2300	41 HV	
HV 0.05	25 to 200	0.2 HV	
HV 0.05	200 to 400	4.6 HV	
HV 0.05	400 to 700	13 HV	
HV 0.05	700 to 2300	29 HV	
HV 0.1	25 to 200	0.2 HV	
HV 0.1	200 to 400	3.3 HV	
HV 0.1	400 to 700	9.2 HV	
HV 0.1	700 to 2300	21 HV	
HV 0.2	25 to 200	0.2 HV	
HV 0.2	200 to 400	2.5 HV	
HV 0.2	400 to 700	6.7 HV	
HV 0.2	700 to 2300	15 HV	
HV 0.3	25 to 200	0.2 HV	
HV 0.3	200 to 400	2.2 HV	
HV 0.3	400 to 700	5.6 HV	
HV 0.3	700 to 2300	13 HV	
HV 0.4	25 to 200	0.2 HV	
HV 0.4	200 to 400	1.9 HV	
HV 0.4	400 to 700	5.0 HV	
HV 0.4	700 to 2300	11 HV	
HV 0.5	25 to 200	0.2 HV	
HV 0.5	200 to 400	1.8 HV	
HV 0.5	400 to 700	4.6 HV	
HV 0.5	700 to 2300	10 HV	
HV 1	25 to 200	0.2 HV	
HV 1	200 to 400	1.5 HV	
HV 1	400 to 700	3.6 HV	
HV 1	700 to 2300	7.7 HV	

2020-09-18 through 2021-09-30

Effective dates



For the National Voluntary Laboratory Accreditation Program

CALIBRATION LABORATORIES


NVLAP LAB CODE 200127-0

CALIBRATION AND MEASUREMENT CAPABILITIES (CMC)^{Notes 1,2,11}

Measured Parameter or Device Calibrated	Range	Expanded Uncertainty^{Note 3}	Remarks
Calibrate Reference Test Blocks and Indenters Knoop: ASTM E384, ISO 4545 Knoop Scale			See notes 7, 8, and 10 Range in Knoop units
HK 0.01	25 to 200	0.5 HK	
HK 0.01	200 to 400	4.9 HK	
HK 0.01	400 to 700	12 HK	
HK 0.01	700 to 2300	24 HK	
HK 0.025	25 to 200	0.5 HK	
HK 0.025	200 to 400	4.2 HK	
HK 0.025	400 to 700	9.4 HK	
HK 0.025	700 to 2300	18 HK	
HK 0.05	25 to 200	0.5 HK	
HK 0.05	200 to 400	3.9 HK	
HK 0.05	400 to 700	8.5 HK	
HK 0.05	700 to 2300	16 HK	
HK 0.1	25 to 200	0.5 HK	
HK 0.1	200 to 400	3.8 HK	
HK 0.1	400 to 700	8.0 HK	
HK 0.1	700 to 2300	15 HK	
HK 0.2	25 to 200	0.5 HK	
HK 0.2	200 to 400	3.8 HK	
HK 0.2	400 to 700	7.7 HK	
HK 0.2	700 to 2300	14 HK	
HK 0.3	25 to 200	0.5 HK	
HK 0.3	200 to 400	3.7 HK	
HK 0.3	400 to 700	7.6 HK	
HK 0.3	700 to 2300	13 HK	
HK 0.5	25 to 200	0.5 HK	
HK 0.5	200 to 400	3.7 HK	
HK 0.5	400 to 700	7.6 HK	
HK 0.5	700 to 2300	13 HK	
HK 1	25 to 200	0.5 HK	
HK 1	200 to 400	3.7 HK	
HK 1	400 to 700	7.5 HK	
HK 1	700 to 2300	13 HK	

2020-09-18 through 2021-09-30

Effective dates



For the National Voluntary Laboratory Accreditation Program

CALIBRATION LABORATORIES


NVLAP LAB CODE 200127-0

CALIBRATION AND MEASUREMENT CAPABILITIES (CMC)^{Notes 1,2,11}

Measured Parameter or Device Calibrated	Range	Expanded Uncertainty^{Note 3}	Remarks	
Direct Verification Brinell Hardness Laboratory Capability ASTM E10, ISO 6506	0 mm to 7 mm	0.0038 mm	Indentation Measurement System	
Direct Verification Vickers Hardness Laboratory Capability ASTM E384, E92, ISO 6507	0 mm to 0.100 mm 1 mm to 0.200 mm	0.0003 mm 0.00036 mm		
Direct Verification Knoop Hardness Laboratory Capability ASTM E384, ISO 4545	0 mm to 0.100 mm 1 mm to 0.200 mm	0.0003 mm 0.00036 mm		
Direct Verification Field Calibration ^{Note 4} Brinell Hardness ASTM E10, ISO 6506	0 mm to 7 mm	0.028 mm		Indentation Measurement System
Direct Verification Field Calibration ^{Note 4} Vickers Hardness ASTM E92, ISO 6507, ASTM E384	0 mm to 0.500 mm	0.0014 mm		
Direct Verification Field Calibration ^{Note 4} Vickers Hardness ASTM E384, ISO 6507	0 mm to 0.200 mm	0.001 mm		
Direct Verification Field Calibration ^{Note 4} Knoop Hardness ASTM E384, ISO 4545	0 mm to 0.200 mm	0.001 mm		

2020-09-18 through 2021-09-30

Effective dates



For the National Voluntary Laboratory Accreditation Program

CALIBRATION LABORATORIES


NVLAP LAB CODE 200127-0

CALIBRATION AND MEASUREMENT CAPABILITIES (CMC)^{Notes 1,2,11}

Measured Parameter or Device Calibrated	Range	Expanded Uncertainty ^{Note 3}	Remarks
Direct Verification Rockwell Hardness Laboratory and Field Calibrations ^{Note 4} ASME E18, ISO 6508	0 mm to 3 mm	0.0003 mm	Direct verification of depth is valid only for United Tru-Blue II testers with a Heidenhain Metro Gage, over temperature range 10 °C to 40 °C
Direct Verification Brinell Hardness Laboratory Capability ASTM E10, ISO 6506	1 kgf 1.25 kgf 2.5 kgf 5 kgf 6.25 kgf 7.81 kgf 10 kgf 15.62 kgf 25 kgf 30 kgf 31.25 kgf 62.5 kgf 100 kgf 125 kgf 187.5 kgf 250 kgf 500 kgf 750 kgf 1000 kgf 1500 kgf 2000 kgf 2500 kgf 3000 kgf	0.01 kgf 0.01 kgf 0.01 kgf 0.02 kgf 0.02 kgf 0.02 kgf 0.03 kgf 0.04 kgf 0.06 kgf 0.08 kgf 0.16 kgf 0.32 kgf 0.25 kgf 0.31 kgf 0.95 kgf 1.3 kgf 2.6 kgf 0.63 kgf 3.6 kgf 5.8 kgf 6.7 kgf 7.8 kgf 9.3 kgf	Applied Force

2020-09-18 through 2021-09-30

Effective dates



For the National Voluntary Laboratory Accreditation Program

CALIBRATION LABORATORIES


NVLAP LAB CODE 200127-0

CALIBRATION AND MEASUREMENT CAPABILITIES (CMC)^{Notes 1,2,11}

Measured Parameter or Device Calibrated	Range	Expanded Uncertainty ^{Note 3}	Remarks
Direct Verification Vickers Hardness Laboratory Capability ASTM E92, ISO 6507, ASTM E384	1 kgf 1.5 kgf 2 kgf 2.5 kgf 3 kgf 5 kgf 10 kgf 20 kgf 30 kgf 50 kgf 100 kgf	0.003 kgf 0.006 kgf 0.006 kgf 0.007 kgf 0.012 kgf 0.02 kgf 0.05 kgf 0.088 kgf 0.13 kgf 0.21 kgf 0.44 kgf	Applied Force
Direct Verification Vickers Hardness Laboratory Capability ASTM E384, ISO 6507	10 gf 25 gf 50 gf 100 gf 200 gf 300 gf 400 gf 500 gf 1000 gf 2000 gf 3000 gf	1 gf 1 gf 1 gf 1 gf 1 gf 2.1 gf 2.1 gf 3.1 gf 5.5 gf 11 gf 16 gf	Applied Force
Direct Verification Knoop Hardness Laboratory Capability ASTM E384, ISO 4545	10 gf 25 gf 50 gf 100 gf 200 gf	1 gf 1 gf 1 gf 1 gf 1 gf	Applied Force

2020-09-18 through 2021-09-30

Effective dates



For the National Voluntary Laboratory Accreditation Program

CALIBRATION LABORATORIES


NVLAP LAB CODE 200127-0

CALIBRATION AND MEASUREMENT CAPABILITIES (CMC)^{Notes 1,2,11}

Measured Parameter or Device Calibrated	Range	Expanded Uncertainty ^{Note 3}	Remarks
Direct Verification Field Calibration ^{Note 4} Brinell Hardness ASTM E10, ISO 6506	300 gf	2.1 gf	Applied Force
	400 gf	2.1 gf	
	500 gf	3.1 gf	
	1000 gf	5.5 gf	
	2000 gf	11 gf	
	3000 gf	16 gf	
Direct Verification Field Calibration ^{Note 4} Vickers Hardness ASTM E92 ISO 6507, ASTM E384	62.5 kgf	0.6 kgf	Applied Force
	187.5 kgf	1.9 kgf	
	500 kgf	5.0 kgf	
	1000 kgf	5.8 kgf	
	1500 kgf	7.4 kgf	
	2000 kgf	8.1 kgf	
	2500 kgf	9.5 kgf	
	3000 kgf	10 kgf	
Field Calibration ^{Note 4} Vickers Hardness ASTM E384, ISO 6507	1 kgf	0.006 kgf	Applied Force
	2 kgf	0.012 kgf	
	5 kgf	0.030 kgf	
	10 kgf	0.060 kgf	
	20 kgf	0.12 kgf	
	30 kgf	0.18 kgf	
Field Calibration ^{Note 4} Vickers Hardness ASTM E384, ISO 6507	50 kgf	0.30 kgf	Applied Force
	10 gf	1 gf	
	25 gf	1 gf	
	50 gf	1 gf	
	100 gf	1 gf	
	200 gf	1 gf	

2020-09-18 through 2021-09-30

Effective dates



For the National Voluntary Laboratory Accreditation Program

CALIBRATION LABORATORIES


NVLAP LAB CODE 200127-0

CALIBRATION AND MEASUREMENT CAPABILITIES (CMC)^{Notes 1,2,11}

Measured Parameter or Device Calibrated	Range	Expanded Uncertainty ^{Note 3}	Remarks		
Field Calibration ^{Note 4} Knoop Hardness ASTM E384, ISO 4545	300 gf	2.1 gf	Applied Force		
	500 gf	3.1 gf			
	1000 gf	5.5 gf			
Rockwell Hardness Testers - Direct Laboratory & Field Calibration ^{Note 4} ASTM E4	10 gf	1 gf			
	25 gf	1 gf			
	50 gf	1 gf			
	100 gf	1 gf			
	200 gf	1 gf			
	300 gf	2.1 gf			
	500 gf	3.1 gf			
	1000 gf	5.5 gf			
Indirect Field Service ^{Note 4} And Laboratory Calibration Brinell Hardness Testers ASTM E10, ISO 6506 Brinell Scale	3 kgf	10 gf	Applied Force		
	10 kgf	10 gf			
	15 kgf	10 gf			
	30 kgf	10 gf			
	45 kgf	10 gf			
	60 kgf	30 gf			
	100 kgf	30 gf			
	150 kgf	30 gf			
	HBW 1/62.5	200 to 400		2 HBW	See notes 7 and 8. Range in Brinell units
		400 to 600		4 HBW	
HBW 2.5/187.5		200 to 400	2 HBW		
400 to 600		4 HBW			
HBW 10/500		20 to 100	2 HBW		
100 to 150		4HBW			
HBW 5/1000		200 to 400	2 HBW		
400 to 600		4 HBW			

2020-09-18 through 2021-09-30

Effective dates



For the National Voluntary Laboratory Accreditation Program

CALIBRATION LABORATORIES


NVLAP LAB CODE 200127-0

CALIBRATION AND MEASUREMENT CAPABILITIES (CMC)^{Notes 1,2,11}

Measured Parameter or Device Calibrated	Range	Expanded Uncertainty ^{Note 3}	Remarks
HBW 10/1000	200 to 400	2 HBW	See notes 7 and 8. Range in Vickers units
HBW 10/1000	400 to 600	4 HBW	
HBW 10/1500	200 to 400	2 HBW	
HBW 10/1500	400 to 600	4 HBW	
HBW 10/2000	200 to 400	2 HBW	
HBW 10/2000	400 to 600	4 HBW	
HBW 10/2500	200 to 400	2 HBW	
HBW 10/2500	400 to 600	4 HBW	
HBW 10/3000	200 to 400	2 HBW	
HBW 10/3000	400 to 600	4 HBW	
Indirect Field Service ^{Note 4} And Laboratory Calibration Vickers Hardness Testers ASTM E92, ISO 6507, ASTM E384 Vickers Scale			
HV 1	200	8.7 HV	
HV 1	400	21 HV	
HV 1	700	44 HV	
HV 2	200	6.9 HV	
HV 2	400	16 HV	
HV 2	700	31 HV	
HV 5	200	3.9 HV	
HV 5	400	11 HV	
HV 5	700	20 HV	
HV 10	200	3.1 HV	
HV 10	400	7.7 HV	
HV 10	700	15 HV	
HV 20	200	2.5 HV	
HV 20	400	6.2 HV	
HV 20	700	11 HV	
HV 30	200	2 HV	
HV 30	400	4.4 HV	
HV 30	700	9.3 HV	
HV 50	200	1.9 HV	

2020-09-18 through 2021-09-30

Effective dates



For the National Voluntary Laboratory Accreditation Program

CALIBRATION LABORATORIES


NVLAP LAB CODE 200127-0

CALIBRATION AND MEASUREMENT CAPABILITIES (CMC)^{Notes 1,2,11}

Measured Parameter or Device Calibrated	Range	Expanded Uncertainty ^{Note 3}	Remarks
HV 50	400	3.5 HV	See notes 7 and 8. Range in Vickers units
HV 50	700	6.3 HV	
Indirect Field Service ^{Note 4} And Laboratory Calibration Vickers Hardness Testers ASTM E384, ISO 6507 Vickers Scale			
HV 0.01	200	10 HV	
HV 0.01	400	30 HV	
HV 0.01	700	40 HV	
HV 0.025	200	9 HV	
HV 0.025	400	20 HV	
HV 0.025	700	30 HV	
HV 0.05	200	8.5 HV	
HV 0.05	400	19 HV	
HV 0.05	700	27 HV	
HV 0.1	200	8 HV	
HV 0.1	400	18 HV	
HV 0.1	700	25 HV	
HV 0.2	200	7 HV	
HV 0.2	400	17 HV	
HV 0.2	700	20 HV	
HV 0.3	200	6 HV	
HV 0.3	400	16 HV	
HV 0.3	700	19 HV	
HV 0.5	200	5 HV	
HV 0.5	400	15 HV	
HV 0.5	700	17 HV	
HV 1	200	5 HV	
HV 1	400	10 HV	
HV 1	700	15 HV	

2020-09-18 through 2021-09-30

Effective dates



For the National Voluntary Laboratory Accreditation Program

CALIBRATION LABORATORIES


NVLAP LAB CODE 200127-0

CALIBRATION AND MEASUREMENT CAPABILITIES (CMC) ^{Notes 1,2,11}

Measured Parameter or Device Calibrated	Range	Expanded Uncertainty ^{Note 3}	Remarks
Indirect Field Service ^{Note 4} And Laboratory Calibration Knoop Hardness Testers ASTM E384, ISO 4545 Knoop Scale			See notes 7 and 8.
HK 0.01	200	7 HK	Range in Knoop units
HK 0.01	400	16 HK	
HK 0.01	700	33 HK	
HK 0.025	200	7 HK	
HK 0.025	400	14 HK	
HK 0.025	700	22 HK	
HK 0.05	200	7 HK	
HK 0.05	400	14 HK	
HK 0.05	700	20 HK	
HK 0.1	200	7 HK	
HK 0.1	400	12 HK	
HK 0.1	700	19 HK	
HK 0.2	200	5 HK	
HK 0.2	400	8 HK	
HK 0.2	700	17 HK	
HK 0.3	200	5 HK	
HK 0.3	400	8 HK	
HK 0.3	700	17 HK	
HK 0.5	200	5 HK	
HK 0.5	400	7 HK	
HK 0.5	700	15 HK	
HK 1	200	5 HK	
HK 1	400	7 HK	
HK 1	700	15 HK	
Calibration of Durometer Blocks ASTM D2240 Hardness scale			
Shore A	0 to 100	0.8	Uncertainty given in Shore units
Shore D	0 to 100	0.8	

2020-09-18 through 2021-09-30

Effective dates



For the National Voluntary Laboratory Accreditation Program

CALIBRATION LABORATORIES


NVLAP LAB CODE 200127-0

CALIBRATION AND MEASUREMENT CAPABILITIES (CMC)^{Notes 1,2,11}

Measured Parameter or Device Calibrated	Range	Expanded Uncertainty ^{Note 3}	Remarks
Calibration of Durometers ASTM D2240 Spring Force Shore A Shore D	0 N to 8.9 N 0 N to 44 N	0.0002 N 0.006 N	Tip shape verified for condition only. Indenter extension verified by use of gage blocks.
Indenter Extension	0 mm to 6.35 mm	0.005 mm	
Calibration of Leeb's Testers ASTM A956	400 LD to 900 LD	8.5 LD	
Calibration of Leeb's Blocks ASTM A956	400 LD to 900 LD	9.3 LD	
END			

2020-09-18 through 2021-09-30

Effective dates



For the National Voluntary Laboratory Accreditation Program

Notes

Note 1: A Calibration and Measurement Capability (CMC) is a description of the best result of a calibration or measurement (result with the smallest uncertainty of measurement) that is available to the laboratory's customers under normal conditions, when performing more or less routine calibrations of nearly ideal measurement standards or instruments. The CMC is described in the laboratory's scope of accreditation by: the measurement parameter/device being calibrated, the measurement range, the uncertainty associated with that range (see note 3), and remarks on additional parameters, if applicable.

Note 2: Calibration and Measurement Capabilities are traceable to the national measurement standards of the U.S. or to the national measurement standards of other countries and are thus traceable to the internationally accepted representation of the appropriate SI (Système International) unit.

Note 3: The uncertainty associated with a measurement in a CMC is an expanded uncertainty with a level of confidence of approximately 95 %, typically using a coverage factor of $k = 2$. However, laboratories may report a coverage factor different than $k = 2$ to achieve the 95 % level of confidence. Units for the measurand and its uncertainty are to match. Exceptions to this occur when marketplace practice employs mixed units, such as when the artifact to be measured is labeled in non-SI units and the uncertainty is given in SI units (Example: 5 lb weight with uncertainty given in mg).

Note 3a: The uncertainty of a specific calibration by the laboratory may be greater than the uncertainty in the CMC due to the condition and behavior of the customer's device and specific circumstances of the calibration. The uncertainties quoted do not include possible effects on the calibrated device of transportation, long term stability, or intended use.

Note 3b: As the CMC represents the best measurement results achievable under normal conditions, the accredited calibration laboratory shall not report smaller uncertainty of measurement than that given in a CMC for calibrations or measurements covered by that CMC.

Note 3c: As described in Note 1, CMCs cover calibrations and measurements that are available to the laboratory's customers under *normal conditions*. However, the laboratory may have the capability to offer special tests, employing special conditions, which yield calibration or measurement results with lower uncertainties. Such special tests are not covered by the CMCs and are outside the laboratory's scope of accreditation. In this case, NVLAP requirements for the labeling, on calibration reports, of results outside the laboratory's scope of accreditation apply. These requirements are set out in Annex A.5 of NIST Handbook 150, Procedures and General Requirements.


Note 4: Uncertainties associated with field service calibration may be greater as they incorporate on-site environmental contributions, transportation effects, or other factors that affect the measurements. (This note applies only if marked in the body of the scope.)

Note 5: Uncertainty values listed with percent (%) are percent of reading or generated value unless otherwise noted.

Note 6: NVLAP accreditation is the formal recognition of specific calibration capabilities. Neither NVLAP nor NIST guarantee the accuracy of individual calibrations made by accredited laboratories.

2020-09-18 through 2021-09-30

Effective dates



For the National Voluntary Laboratory Accreditation Program

Notes

Note 7: Standardized test blocks used for verification are calibrated at the David L. Ellis Company, Inc. Hardness Calibration Laboratory in accordance with ASTM E10, E18, E92, E384, or ISO 4545, 6506, 6507, 6508 using NIST HRC Standard Reference Materials (SRM) 2810, 2811, 2812 and other primary reference standards from other National Metrology Institutes. Some Rockwell scales are traceable to David L. Ellis Co., Inc. hardness levels through laboratory standardizing machines. These standardizing machines are directly verified according to applicable ASTM or ISO procedures using devices that are traceable to NIST either directly or through a NVLAP-accredited laboratory.

Note 8: Where available, certified materials (NIST (USA), PTB (Germany), and IMGC (Italy)) are used to indirectly verify scales and hardness levels. All other scales and hardness ranges are traceable to directly verified testers with parameters traceable to NIST.


Note 9: The best uncertainty is shown at the highest part of the range and increases as Rockwell value decreases. The uncertainty of the lowest value in the range is equal to the uncertainty listed in the next lower range. Best uncertainty remains the same for all values higher than the ranges shown in each scale.

Note 10: The best uncertainty is shown for the lowest value in the range. The uncertainty increases in a non-linear manner to a value which equals the uncertainty of the next range. The highest value of uncertainty for the upper value is 2 to 3 times higher than value shown depending on type. Please contact the lab for a better estimation of uncertainty for these higher values.

Note 11: Calibrations for Rockwell hardness are performed at either David L. Ellis's Acton facility or their Maynard facility. Other calibrations are performed at Maynard only. Location of specific calibration will be noted on calibration certificate.

2020-09-18 through 2021-09-30

Effective dates

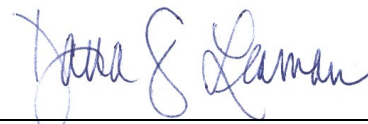

For the National Voluntary Laboratory Accreditation Program